

WATER SUPPLY

Matrices with low concentrations of analytes for testing water supply, drinking water, or ground water. Standards are based on requirements of the United States Environmental Protection Agency Safe Drinking Water Act and may be used to satisfy PT requirements worldwide.



2015 Water Supply PT Scheme Schedule

| | Scheme # | Opens | Closes |
|----------|----------|-------|--------------|
| Q | WS 222 | Jan 5 | Feb 19 |
| | WS 223 | Feb 9 | Mar 26 |
| | WS 224 | Mar 2 | Apr 16 |
| Q | WS 225 | Apr 6 | May 21 |
| | WS 226 | May 4 | Jun 18 |
| | WS 227 | Jun 8 | Jul 23 |
| Q | WS 228 | Jul 6 | Aug 20 |
| | WS 229 | Aug 3 | Sep 17 |
| | WS 230 | Sep 8 | Oct 23 |
| Q | WS 231 | Oct 5 | Nov 19 |
| | WS 232 | Nov 6 | Dec 21 |
| | WS 233 | Dec 7 | Jan 21, 2016 |

Schedule subject to change – see ERA's website at www.eraqc.com

2016 Water Supply PT Scheme Schedule

| | Scheme # | Opens | Closes |
|----------|----------|--------|--------------|
| Q | WS 234 | Jan 11 | Feb 25 |
| | WS 235 | Feb 8 | Mar 24 |
| | WS 236 | Mar 1 | Apr 15 |
| Q | WS 237 | Apr 4 | May 19 |
| | WS 238 | May 9 | Jun 23 |
| | WS 239 | Jun 6 | Jul 21 |
| Q | WS 240 | Jul 11 | Aug 25 |
| | WS 241 | Aug 8 | Sep 22 |
| | WS 242 | Sep 6 | Oct 21 |
| Q | WS 243 | Oct 7 | Nov 21 |
| | WS 244 | Nov 1 | Dec 16 |
| | WS 245 | Dec 5 | Jan 19, 2017 |

Schedule subject to change – see ERA's website at www.eraqc.com

| Description | CRM | PT | QR | Page |
|---|------|---------------|--------|------|
| Carbamates/ Carbamoyloxime Pesticides | 707 | 846 M | 707QR | 36 |
| Chloral Hydrate | 676 | 853 *M | 676QR | 35 |
| Chlordane | 705 | 845 M | 705QR | 36 |
| Chlorinated Acid Herbicides | 704 | 851 M | 704QR | 37 |
| Color | 661 | 859 Q | 661QR | 34 |
| Corrosivity | 980 | 900 Q | 980QR | 34 |
| Cyanide | 983 | 556 M | 983QR | 34 |
| Dioxin | 663 | 857 Q | 663QR | 37 |
| EDB/DBCP/TCP | 706 | 847 M | 706QR | 36 |
| Gasoline Additives | 909 | 905 Q | 909QR | 35 |
| Hardness | 693 | 555 M | 693QR | 32 |
| Haloacetic Acids (HAA) | 684 | 852 M | 684QR | 35 |
| Halomethanes (THMs) | 702 | 842 M | 702QR | 35 |
| Hexavalent Chromium | 658 | 854 Q | 658QR | 32 |
| Inorganics | 698 | 591 M | 698QR | 32 |
| Inorganic Disinfection #1 | 5272 | 5270 M | 5272QR | 33 |
| Inorganic Disinfection #2 | 5262 | 5260 M | 5262QR | 33 |
| Mercury | 666 | 551 M | 666QR | 32 |
| Metals | 697 | 590 M | 697QR | 32 |

CRM – Certified Reference Material

PT – Proficiency Testing

QR – QuiK Response

All ERA WS PTs open monthly (**M**) or quarterly (**Q**) unless otherwise noted.

***M** ERA Chloral Hydrate PTs open in January and July.

Quarterly months are January, April, July, and October.

| Description | CRM | PT | QR | Page |
|--------------------------------|------|---------------|--------|------|
| Nitrite | 695 | 594 M | 695QR | 33 |
| Organic Carbon | 669 | 557 M | 669QR | 34 |
| o-Phosphate Nutrients | 667 | 558 M | 667QR | 33 |
| PCBs as Decachlorobiphenyl | 708 | 839 Q | 708QR | 37 |
| Perchlorate | 910 | 903 Q | 910QR | 34 |
| Pesticides | 709 | 850 M | 709QR | 36 |
| pH | 779 | 552 M | 779QR | 32 |
| Regulated Volatiles | 703 | 840 M | 703QR | 35 |
| Residual Chlorine | 696 | 593 M | 696QR | 34 |
| Semivolatiles #1 | 690 | 848 M | 690QR | 37 |
| Semivolatiles #2 Herbicides | 691 | 849 M | 691QR | 37 |
| Silica | 785 | 902 Q | 785QR | 34 |
| Solids Concentrate | 5152 | 5150 M | 5152QR | 32 |
| Surfactants-MBAS | 784 | 901 Q | 784QR | 34 |
| Toxaphene | 700 | 844 M | 700QR | 36 |
| Turbidity | 699 | 592 M | 699QR | 34 |
| Unregulated Volatiles | 683 | 841 M | 683QR | 35 |
| Uranium | 930 | 858 Q | 930QR | 32 |
| UV 254 Absorbance | 662 | 904 Q | 662QR | 34 |
| Vanadium | 660 | 856 Q | 660QR | 32 |

QuiK Response PT

Need PT results fast? Available 52 weeks a year, QuiK Response PTs are on demand PTs that return final results within minutes of submitting your data online. In the US, please call ERA customer service at 800-372-0122 or 303-431-8454 to order. Outside of the US, please contact your authorized ERA sales partner to order.

MINERALS/SOLIDS

Hardness

| CRM Cat. #693 | PT M Cat. #555 | QR Cat. #693QR |
|------------------|-------------------|-------------------|
|------------------|-------------------|-------------------|

One 250 mL whole-volume bottle is ready to analyze.

| | |
|---|-------------|
| Calcium | 30-90 mg/L |
| Calcium hardness as CaCO ₃ | 75-225 mg/L |
| Total hardness as CaCO ₃ | 83-307 mg/L |
| Magnesium..... | 2-20 mg/L |
| Sodium..... | 12-50 mg/L |

Inorganics

| CRM Cat. #698 | PT M Cat. #591 | QR Cat. #698QR |
|------------------|-------------------|-------------------|
|------------------|-------------------|-------------------|

One 500 mL whole-volume bottle is ready to analyze. The CRM is also certified for Sodium. For a Sodium PT, order Hardness, Cat. #555.

| | |
|---|--------------------|
| Alkalinity as CaCO ₃ | 25-200 mg/L |
| Chloride..... | 20-160 mg/L |
| Fluoride..... | 1-8 mg/L |
| Nitrate as N..... | 3-10 mg/L |
| Nitrate plus nitrite as N..... | 3-10 mg/L |
| Potassium..... | 10-40 mg/L |
| Specific conductance at 25 °C..... | 130-1,300 µmhos/cm |
| Sulfate..... | 25-250 mg/L |
| Total dissolved solids (TDS) at 180 °C..... | 100-1,000 mg/L |

pH

| CRM Cat. #779 | PT M Cat. #552 | QR Cat. #779QR |
|------------------|-------------------|-------------------|
|------------------|-------------------|-------------------|

One 250 mL whole-volume bottle is ready to analyze.

| | |
|---------|------------|
| pH..... | 5-10 units |
|---------|------------|

Solids Concentrate

| CRM Cat. #5152 | PT M Cat. #5150 | QR Cat. #5152QR |
|-------------------|--------------------|--------------------|
|-------------------|--------------------|--------------------|

One 24 mL screw-cap vial with a powder yields 1 liter after dilution.

| | |
|---|----------------|
| Total filterable residue (TDS) at 180 °C..... | 100-1,000 mg/L |
| Total solids (TS) at 105 °C..... | 123-1,100 mg/L |
| Total suspended solids (TSS)..... | 23-100 mg/L |

TRACE METALS

Metals

| CRM Cat. #697 | PT M Cat. #590 | QR Cat. #697QR |
|------------------|-------------------|-------------------|
|------------------|-------------------|-------------------|

One 15 mL screw-cap vial yields up to 2 liters after dilution. Use with ICP-OES, ICP-MS and AA methods.

| | |
|-----------------|----------------|
| Aluminum | 130-1,000 µg/L |
| Antimony..... | 6-50 µg/L |
| Arsenic..... | 5-50 µg/L |
| Barium..... | 500-3,000 µg/L |
| Beryllium..... | 2-20 µg/L |
| Boron..... | 800-2,000 µg/L |
| Cadmium..... | 2-50 µg/L |
| Chromium..... | 10-200 µg/L |
| Copper..... | 50-2,000 µg/L |
| Iron..... | 100-1,800 µg/L |
| Lead..... | 5-100 µg/L |
| Manganese..... | 40-900 µg/L |
| Molybdenum..... | 15-130 µg/L |
| Nickel..... | 10-500 µg/L |
| Selenium..... | 10-100 µg/L |
| Silver..... | 20-300 µg/L |
| Thallium..... | 2-10 µg/L |
| Vanadium..... | 50-1,000 µg/L |
| Zinc..... | 200-2,000 µg/L |

Mercury

| CRM Cat. #666 | PT M Cat. #551 | QR Cat. #666QR |
|------------------|-------------------|-------------------|
|------------------|-------------------|-------------------|

One 15 mL screw-cap vial yields up to 1 liter after dilution. Use with CVAA, ICP-MS or CVAFS methods.

| | |
|---------------------|-------------|
| Mercury, total..... | 0.5-10 µg/L |
|---------------------|-------------|

Hexavalent Chromium

| CRM Cat. #658 | PT Q Cat. #854 | QR Cat. #658QR |
|------------------|-------------------|-------------------|
|------------------|-------------------|-------------------|

One 15 mL screw-cap vial yields up to 2 liters after dilution.

| | |
|--------------------------|-----------|
| Hexavalent chromium..... | 5-50 µg/L |
|--------------------------|-----------|

Uranium

| CRM Cat. #930 | PT Q Cat. #858 | QR Cat. #930QR |
|------------------|-------------------|-------------------|
|------------------|-------------------|-------------------|

One 15 mL screw-cap vial yields up to 2 liters after dilution. Use with ICP-MS methods.

| | |
|--------------|------------|
| Uranium..... | 3-104 µg/L |
|--------------|------------|

Vanadium

| CRM Cat. #660 | PT Q Cat. #856 | QR Cat. #660QR |
|------------------|-------------------|-------------------|
|------------------|-------------------|-------------------|

One 15 mL screw-cap vial yields up to 2 liters after dilution. Designed to meet California ELAP requirements.

| | |
|---------------|-----------|
| Vanadium..... | 5-50 µg/L |
|---------------|-----------|

The Industry Standard



DISINFECTION BY-PRODUCTS

Inorganic Disinfection #1

| CRM | PT ^M | QR |
|------------|-----------------|--------------|
| Cat. #5272 | Cat. #5270 | Cat. #5272QR |

One 24 mL screw-cap vial yields up to 4 liters after dilution.

| | |
|---------------|----------------|
| Chlorate..... | 60-180 µg/L |
| Chlorite..... | 100-1,000 µg/L |

Inorganic Disinfection #2

| CRM | PT ^M | QR |
|------------|-----------------|--------------|
| Cat. #5262 | Cat. #5260 | Cat. #5262QR |

One 24 mL screw-cap vial yields up to 4 liters after dilution.

| | |
|--------------|-------------|
| Bromate..... | 7-50 µg/L |
| Bromide..... | 50-300 µg/L |

NUTRIENTS

Nitrite

| CRM | PT ^M | QR |
|-----------|-----------------|-------------|
| Cat. #695 | Cat. #594 | Cat. #695QR |

One 15 mL screw-cap vial yields up to 2 liters after dilution.


| | |
|-------------------|------------|
| Nitrite as N..... | 0.4-2 mg/L |
|-------------------|------------|

o-Phosphate Nutrients

| CRM | PT ^M | QR |
|-----------|-----------------|-------------|
| Cat. #667 | Cat. #558 | Cat. #667QR |

One 15 mL screw-cap vial yields up to 2 liters after dilution.

| | |
|---------------------------|--------------|
| ortho-Phosphate as P..... | 0.5-5.5 mg/L |
|---------------------------|--------------|

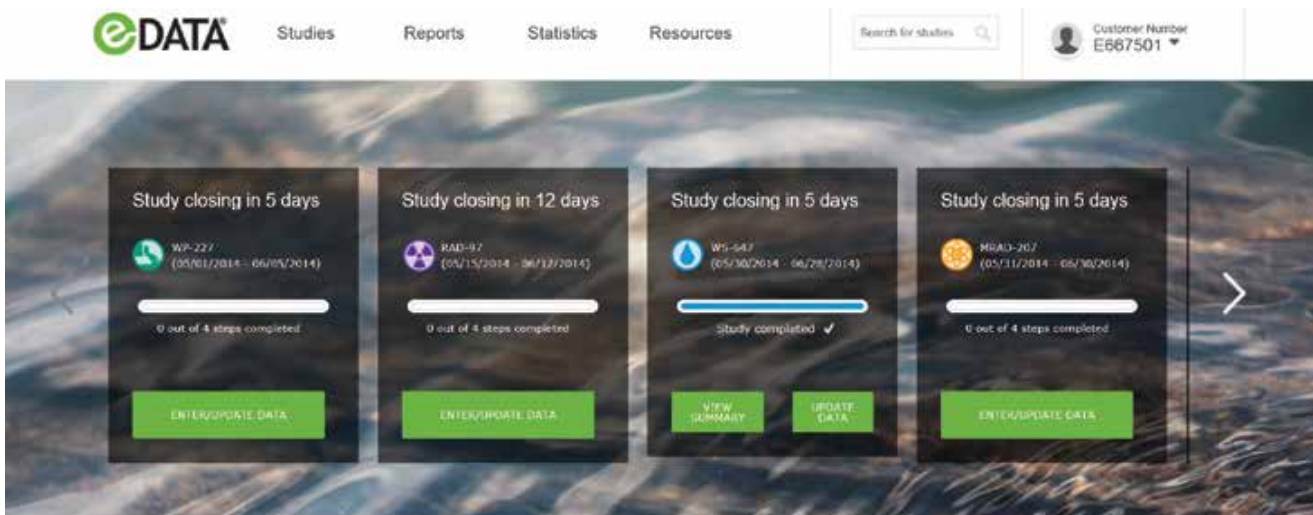

eDATA 2.0: New in 2015

Effortless Insight

- Save time and money with ultra-fast, streamlined data entry.
- Easily identify problems to take corrective action with empowering performance evaluation tools.
- Showcase your quality with innovative performance reports for your laboratory or entire network.
- Effortlessly understand your entire network's performance with specialized tools for corporate managers.
- Eliminate transcription errors and increase productivity by uploading directly from your LIMS.

To learn more, visit www.eraqc.com/resources/edata

All ERA WS PTs open monthly (^M) or quarterly (^Q) unless otherwise noted.

MISCELLANEOUS INORGANIC

Residual Chlorine

| | | |
|-------------------------|--------------------------|--------------------------|
| CRM Cat. #696 | PT M Cat. #593 | QR Cat. #696QR |
|-------------------------|--------------------------|--------------------------|

One 2 mL flame-sealed ampule yields up to 2 liters after dilution.

| | |
|------------------------------|------------|
| Total Residual Chlorine..... | 0.5-3 mg/L |
| Free Residual Chlorine..... | 0.5-3 mg/L |

Cyanide

| | | |
|-------------------------|--------------------------|--------------------------|
| CRM Cat. #983 | PT M Cat. #556 | QR Cat. #983QR |
|-------------------------|--------------------------|--------------------------|

One 15 mL screw-cap vial yields up to 2 liters after dilution. Source material is free cyanide.

| | |
|--------------------|--------------|
| Total Cyanide..... | 0.1-0.5 mg/L |
|--------------------|--------------|

Organic Carbon

| | | |
|-------------------------|--------------------------|--------------------------|
| CRM Cat. #669 | PT M Cat. #557 | QR Cat. #669QR |
|-------------------------|--------------------------|--------------------------|

One 15 mL screw-cap vial yields up to 1 liter after dilution.

| | |
|-------------------------------|-------------|
| Total Organic Carbon..... | 1.3-13 mg/L |
| Dissolved Organic Carbon..... | 1.3-13 mg/L |

Perchlorate

| | | |
|-------------------------|--------------------------|--------------------------|
| CRM Cat. #910 | PT Q Cat. #903 | QR Cat. #910QR |
|-------------------------|--------------------------|--------------------------|

One 15 mL screw-cap vial yields up to 2 liters after dilution.

| | |
|------------------|-----------|
| Perchlorate..... | 4-20 µg/L |
|------------------|-----------|

Silica

| | | |
|-------------------------|--------------------------|--------------------------|
| CRM Cat. #785 | PT Q Cat. #902 | QR Cat. #785QR |
|-------------------------|--------------------------|--------------------------|

One 60 mL poly bottle yields 1 liter after dilution.

| | |
|----------------------------------|-----------|
| Silica as SiO ₂ | 5-75 mg/L |
|----------------------------------|-----------|

Surfactants-MBAS

| | | |
|-------------------------|--------------------------|--------------------------|
| CRM Cat. #784 | PT Q Cat. #901 | QR Cat. #784QR |
|-------------------------|--------------------------|--------------------------|

One 15 mL screw-cap vial yields up to 2 liters after dilution.

| | |
|-----------------------|------------|
| Surfactants-MBAS..... | 0.1-1 mg/L |
|-----------------------|------------|

PHYSICAL PROPERTY

Color

| | | |
|-------------------------|--------------------------|--------------------------|
| CRM Cat. #661 | PT Q Cat. #859 | QR Cat. #661QR |
|-------------------------|--------------------------|--------------------------|

One 125 mL whole-volume bottle is ready to analyze.

| | |
|------------|----------------|
| Color..... | 10-75 PC units |
|------------|----------------|

Corrosivity

| | | |
|-------------------------|--------------------------|--------------------------|
| CRM Cat. #980 | PT Q Cat. #900 | QR Cat. #980QR |
|-------------------------|--------------------------|--------------------------|

One 500 mL whole-volume bottle is ready to analyze for corrosivity, calcium carbonate saturation and Langelier saturation index.

| | |
|------------------|-------------------|
| Corrosivity..... | -4 to +4 SI units |
|------------------|-------------------|

Turbidity

| | | |
|-------------------------|--------------------------|--------------------------|
| CRM Cat. #699 | PT M Cat. #592 | QR Cat. #699QR |
|-------------------------|--------------------------|--------------------------|

One 15 mL screw-cap vial yields up to 1 liter after dilution. Use with nephelometric methods.

| | |
|----------------|-----------|
| Turbidity..... | 0.5-8 NTU |
|----------------|-----------|

UV 254 Absorbance

| | | |
|-------------------------|--------------------------|--------------------------|
| CRM Cat. #662 | PT Q Cat. #904 | QR Cat. #662QR |
|-------------------------|--------------------------|--------------------------|

One 15 mL screw-cap vial yields up to 1 liter after dilution.

| | |
|------------------------|---------------------------|
| UV 254 Absorbance..... | 0.05-0.7 cm ⁻¹ |
|------------------------|---------------------------|

DISINFECTION BY-PRODUCTS

Chloral Hydrate

| CRM | PT* | QR |
|-----------|-----------|-------------|
| Cat. #676 | Cat. #853 | Cat. #676QR |

One 2 mL flame-sealed ampule yields in excess of 200 mL after dilution. Use with EPA method 551, or other applicable method. Includes chloral hydrate at 4-30 µg/L.

* ERA WS Chloral Hydrate PTs open in January and July.

Haloacetic Acids (HAA)

| CRM | PT M | QR |
|-----------|-----------|-------------|
| Cat. #684 | Cat. #852 | Cat. #684QR |

One 2 mL flame-sealed ampule yields up to 2 liters after dilution. Use with EPA method 552, or other applicable method. Includes all the analytes below at 5-50 µg/L.

| | | |
|------------------------|----------------------|-----------------------|
| Bromochloroacetic Acid | Dichloroacetic Acid | Monochloroacetic Acid |
| Dibromoacetic Acid | Monobromoacetic Acid | Trichloroacetic Acid |

VOLATILE ORGANICS

Gasoline Additives

| CRM | PT Q | QR |
|-----------|-----------|-------------|
| Cat. #909 | Cat. #905 | Cat. #909QR |

One 2 mL flame-sealed ampule yields in excess of 200 mL after dilution. Use with EPA method 524.2, or other applicable method for gasoline additives/oxygenates. Contains all of the analytes below at 5-50 µg/L.

| | | |
|-------------------------------|--------------------------------|--------------------------|
| tert-Amyl methyl ether (TAME) | Ethyl tert-butyl ether (ETBE) | Trichlorofluoromethane |
| tert-Butyl Alcohol | Methyl tert-butyl ether (MTBE) | (Freon® 11) |
| Di-isopropylether (DIPE) | | Trichlorotrifluoroethane |
| | | (Freon 113) |

Halomethanes (THMs)

| CRM | PT M | QR |
|-----------|-----------|-------------|
| Cat. #702 | Cat. #842 | Cat. #702QR |

One 2 mL flame-sealed ampule yields in excess of 200 mL after dilution. Use with EPA methods 502.2, 524.2, 551, or other applicable method. Contains all of the analytes below at 5-50 µg/L.

| | | |
|----------------------|----------------------|------------|
| Bromodichloromethane | Chlorodibromomethane | Chloroform |
| Bromoform | | |

Regulated Volatiles

| CRM | PT M | QR |
|-----------|-----------|-------------|
| Cat. #703 | Cat. #840 | Cat. #703QR |

One 2 mL flame-sealed ampule yields in excess of 200 mL after dilution. Use with EPA methods 502.2, 524.2, or other applicable method. Contains all of the analytes below at 2-50 µg/L.

| | | |
|----------------------|----------------------------|------------------------|
| Benzene | cis-1,2-Dichloroethylene | Toluene |
| Carbon tetrachloride | trans-1,2-Dichloroethylene | 1,2,4-Trichlorobenzene |
| Chlorobenzene | 1,2-Dichloropropane | 1,1,1-Trichloroethane |
| 1,2-Dichlorobenzene | Ethylbenzene | 1,1,2-Trichloroethane |
| 1,4-Dichlorobenzene | Methylene chloride | Trichloroethylene |
| 1,2-Dichloroethane | Styrene | Vinyl chloride |
| 1,1-Dichloroethylene | Tetrachloroethylene | Xylenes, total |

Unregulated Volatiles

| CRM | PT M | QR |
|-----------|-----------|-------------|
| Cat. #683 | Cat. #841 | Cat. #683QR |

One 2 mL flame-sealed ampule yields in excess of 200 mL after dilution. Use with EPA methods 502.2, 524.2, or other applicable method. Contains at least 60% of the analytes randomly selected from the list below at 2-50 µg/L.

| | | |
|--------------------|---------------------------|--------------------------------|
| Bromobenzene | 1,3-Dichlorobenzene | 4-Isopropyltoluene |
| Bromochloromethane | Dichlorodifluoromethane | Methyl tert-butyl ether (MTBE) |
| Bromomethane | 1,1-Dichloroethane | Naphthalene |
| n-Butylbenzene | 1,3-Dichloropropane | n-Propylbenzene |
| sec-Butylbenzene | 2,2-Dichloropropane | 1,1,1,2-Tetrachloroethane |
| tert-Butylbenzene | 1,1-Dichloropropene | 1,1,2,2-Tetrachloroethane |
| Chloroethane | cis-1,3-Dichloropropene | 1,2,3-Trichlorobenzene |
| Chloromethane | trans-1,3-Dichloropropene | 1,2,3-Trichloropropane |
| 2-Chlorotoluene | Fluorotrichloromethane | 1,2,4-Trimethylbenzene |
| 4-Chlorotoluene | Hexachlorobutadiene | 1,3,5-Trimethylbenzene |
| Dibromomethane | Isopropylbenzene | |

All ERA WS PTs open monthly (M) or quarterly (Q) unless otherwise noted.

PESTICIDES

Pesticides

| CRM | PT M | QR |
|-----------|-----------|-------------|
| Cat. #709 | Cat. #850 | Cat. #709QR |

One 2 mL flame-sealed ampule yields up to 2 liters after dilution. Use with EPA methods 505, 507, 508, 525, or other applicable method for organochlorine, nitrogen, and organophosphorus pesticides. Each standard contains at least 14 analytes randomly selected from the list below at 0.2-20 µg/L.

| | | |
|-----------|---------------------------|-------------------|
| Alachlor | Heptachlor | Metribuzin |
| Aldrin | Heptachlor epoxide (beta) | Molinate (Ordram) |
| Atrazine | Hexachlorobenzene | Prometon |
| Bromacil | Hexachlorocyclopentadiene | Propachlor |
| Butachlor | Lindane (gamma-BHC) | Simazine |
| Diazinon | Methoxychlor | Thiobencarb |
| Dieldrin | Metolachlor | Trifluralin |
| Endrin | | |

Chlordane

| CRM | PT M | QR |
|-----------|-----------|-------------|
| Cat. #705 | Cat. #845 | Cat. #705QR |

One 2 mL flame-sealed ampule yields up to 2 liters after dilution. Use with EPA methods 505, 508, 525, or other applicable method. Each standard contains technical chlordane at 2-20 µg/L.

Toxaphene

| CRM | PT M | QR |
|-----------|-----------|-------------|
| Cat. #700 | Cat. #844 | Cat. #700QR |

One 2 mL flame-sealed ampule yields up to 2 liters after dilution. Use with EPA methods 505, 508, 525, or other applicable method. Each standard contains toxaphene at 2-20 µg/L.

Meet the Experts Webinar Series

Monthly webcast by our senior scientists designed to help you:

- Ensure your successful Proficiency Testing performance
- Solve routine analysis challenges
- Improve root cause analysis and corrective action

Register via our bi-monthly e-newsletter or webinar invitation via e-mail.

For more information or to view our previously recorded webinars, visit

www.eraqc.com/resources/webinars

Carbamate/Carbamoyloxime Pesticides

| CRM | PT M | QR |
|-----------|-----------|-------------|
| Cat. #707 | Cat. #846 | Cat. #707QR |

One 2 mL flame-sealed ampule yields up to 2 liters after dilution. Use with EPA methods 531.1, 531.2, 632, or other applicable method. Each standard contains at least 8 of the analytes below at 15-150 µg/L.

| | | |
|--------------------|---------------------|------------|
| Aldicarb | Carbaryl | Methiocarb |
| Aldicarb sulfone | Carbofuran | Methomyl |
| Aldicarb sulfoxide | 3-Hydroxycarbofuran | Oxamyl |
| Baygon | | |

EDB/DBCP/TCP

| CRM | PT M | QR |
|-----------|-----------|-------------|
| Cat. #706 | Cat. #847 | Cat. #706QR |

One 2 mL flame-sealed ampule yields in excess of 200 mL after dilution. Use with EPA methods 504, 551, or other applicable method. Each lot contains all analytes below at 0.05-2 µg/L.

| |
|------------------------------------|
| 1,2-Dibromo-3-Chloropropane (DBCP) |
| Ethylene dibromide (EDB) |
| 1,2,3-Trichloropropane (1,2,3-TCP) |

SEMIVOLATILE ORGANICS

Dioxin

| CRM | PT Q | QR |
|-----------|-------------|-------------|
| Cat. #663 | Cat. #857 | Cat. #663QR |

One 2 mL flame-sealed ampule yields up to 2 liters after dilution. Use with EPA methods 613, 1613, 8280, 8290, or other applicable method. Each standard contains 2,3,7,8-TCDD at 20-100 µg/L.

PCBs as Decachlorobiphenyl

| CRM | PT Q | QR |
|-----------|-------------|-------------|
| Cat. #708 | Cat. #839 | Cat. #708QR |

One 2 mL flame-sealed ampule yields up to 2 liters after dilution. Use with EPA quantitative method 508A. This standard can also be used for Aroclor identification and quantification using EPA methods 505, 508, 508.1, or other applicable method. Includes an Aroclor randomly selected from the list below at 0.5-5 µg/L as decachlorobiphenyl.

| | | |
|--------------|--------------|--------------|
| Aroclor 1016 | Aroclor 1242 | Aroclor 1254 |
| Aroclor 1221 | Aroclor 1248 | Aroclor 1260 |
| Aroclor 1232 | | |

Semivolatiles #1

| CRM | PT M | QR |
|-----------|-------------|-------------|
| Cat. #690 | Cat. #848 | Cat. #690QR |

One 2 mL flame-sealed ampule yields up to 2 liters after dilution. Use with EPA methods 506, 525, 550, or other applicable method for PAHs, phthalates and adipates. Each standard contains Benzo(a)pyrene, Bis(2-ethylhexyl)adipate, and Bis(2-ethylhexyl)phthalate plus at least 13 additional analytes, selected from the list below, at 0.2-50 µg/L.

| | | |
|----------------------|--------------------------|----------------------------|
| Acenaphthene | Butyl benzyl phthalate | bis(2-Ethylhexyl)phthalate |
| Acenaphthylene | Chrysene | Fluoranthene |
| Anthracene | Dibenz(a,h)anthracene | Fluorene |
| Benzo(a)anthracene | Di-n-butyl phthalate | Indeno(1,2,3-cd)pyrene |
| Benzo(b)fluoranthene | Diethyl phthalate | Naphthalene |
| Benzo(k)fluoranthene | Dimethyl phthalate | Phenanthrene |
| Benzo(g,h,i)perylene | Di-n-octyl phthalate | Pyrene |
| Benzo(a)pyrene | bis(2-Ethylhexyl)adipate | |

Naphthalene is not within the EPA/NELAC range. Use the Unregulated Volatiles standard (page 35) for this compound in the EPA/NELAC range.

HERBICIDES

Chlorinated Acid Herbicides

| CRM | PT M | QR |
|-----------|-------------|-------------|
| Cat. #704 | Cat. #851 | Cat. #704QR |

One 2 mL flame-sealed ampule yields up to 2 liters after dilution. Use with EPA methods 515.1, 515.2, 515.3, 515.4, 555, or other applicable method. All lots include at least 10 analytes from the list below at 1-120 µg/L.

| | | |
|-----------------------|--------------------------|-------------------|
| Acifluorfen | Dalapon | 4-Nitrophenol |
| Bentazone | Dicamba | Pentachlorophenol |
| Chloramben | 3,5-Dichlorobenzoic acid | Picloram |
| 2,4-D | Dichlorprop | 2,4,5-T |
| 2,4-DB | Dinoseb | 2,4,5-TP (Silvex) |
| Dacthal diacid (DCPA) | | |

Semivolatiles #2 Herbicides

| CRM | PT M | QR |
|-----------|-------------|-------------|
| Cat. #691 | Cat. #849 | Cat. #691QR |

One 2 mL flame-sealed ampule yields up to 2 liters after dilution. Use with EPA methods 547, 548, 549, or other applicable method. Each standard contains all the analytes below at 8-800 µg/L.

| | | |
|-----------|------------|----------|
| Diquat | Glyphosate | Paraquat |
| Endothall | | |



CUSTOMERS ARE RESPONDING ABOUT FASTER PT RESULTS...

“Quick feedback is always good. Confirms a job well done for lab staff and allows for quick troubleshooting if there was a problem identified.”

- Lab Manager, Tennessee

All ERA WS PTs open monthly (**M**) or quarterly (**Q**) unless otherwise noted.

US [T] 800.372.0122 (or) 303.431.8454 [E] info@eraqc.com UK [T] +44 (0) 161 946 2777 [E] sales@eraqc.com